



Client: ACCESS MEDICAL LABORATORI 1 5151 CORPORATE WAY JUPITER, FL 33458	Patient: TEST, PATIENT Room# DOB. 02/05/1985 Age:34 Sex:F Phone: () - Fasting: N ID#: A1909001657780 Route#: 0
Phys: SARA, ALAN (561) 745-1233	Page:1

Acc# 001657780	Coll. Date: 09/11/19	Recv. Date: 09/11/19	Print Date: 09/11/19
Chart#	Coll. Time: 00:00 AM	Recv. Time:12:12 PM	Print Time: 13:09
First reported on:	09/11/19	Final report date:	09/11/19

Test Name	Results	Normal Range	Units
-----------	---------	--------------	-------

Report Status: FINAL

COMMENTS:

Results created randomly. Not real results.

**FEMALE HORMONE PANELS
COMP FEMALE PANEL, SALIVA**

ESTRONE, SALIVA (E1), AM 5.0 <16.0 pg/ml
ESTRADIOL, SALIVA (E2),AM 5.1 pg/ml

PREMENOPAUSAL - Luteal 0.2-5.2 pg/ml
PREMENOPAUSAL - Follicular 0.2-4.0 pg/ml
POSTMENOPAUSAL <2.7 pg/ml
ESTROGEN Replacement (Cream) >5.0 pg/ml
Synthetic HRT, or Contraceptive, is not measured.

ESTRIOL, SALIVA (E3), AM 10.0 pg/ml

Pre-and Postmenopausal < 12.0 pg/mL
Topical Estriol, Bi-Triest therapy > 10.0 pg/mL

PROGESTERONE, SALIVA, AM 88 pg/ml

Premenopausal-Luteal 80 - 270 pg/mL
Premenopausal-Follicular 12 - 100 pg/mL
Postmenopausal 5 - 100 pg/mL
Topical, Troche, Vaginal >200 pg/mL

Synthetic Progestins are not measured. We measure Bioidentical Hormones.

TESTOSTERONE, SALIVA, AM 18 4 - 33 pg/ml
MELATONIN, SALIVA, AM 5.5 0.1 - 25.0 pg/ml

(Continued on Next Page)



Client: ACCESS MEDICAL LABORATORI 1 5151 CORPORATE WAY JUPITER, FL 33458	Patient: TEST, PATIENT Room# _____ DOB. 02/05/1985 Age:34 Sex:F Phone: () - _____ Fasting: N ID#: A1909001657780 Route#: 0
Phys: SARA, ALAN (561) 745-1233	Page:2

Acc# 001657780	Coll. Date: 09/11/19	Recv. Date: 09/11/19	Print Date: 09/11/19
Chart#	Coll. Time: 00:00 AM	Recv. Time:12:12 PM	Print Time: 13:09
First reported on:	09/11/19	Final report date:	09/11/19

Test Name	Results	Normal Range	Units
-----------	---------	--------------	-------

FEMALE HORMONE PANELS (Continued)

CORTISOL, SALIVA, AM	3.25	1.8 - 3.8	ng/ml
DHEA, SALIVA, AM	0.35	0.10 - 1.30	ng/ml


INDIVIDUAL SALIVA TESTS

Progesterone/Estradiol Ra	17 L	45 - 450
Lab Developed Tests	*****	

All Saliva Testing was developed and its performance characteristics determined by Access Medical Laboratories. It has not been cleared or approved by the FDA. The laboratory is regulated under CLIA and qualified to perform high-complexity testing. These tests are used for clinical purposes. It should not be regarded as investigational or for research.

END OF REPORT

HORMONE CASCADE

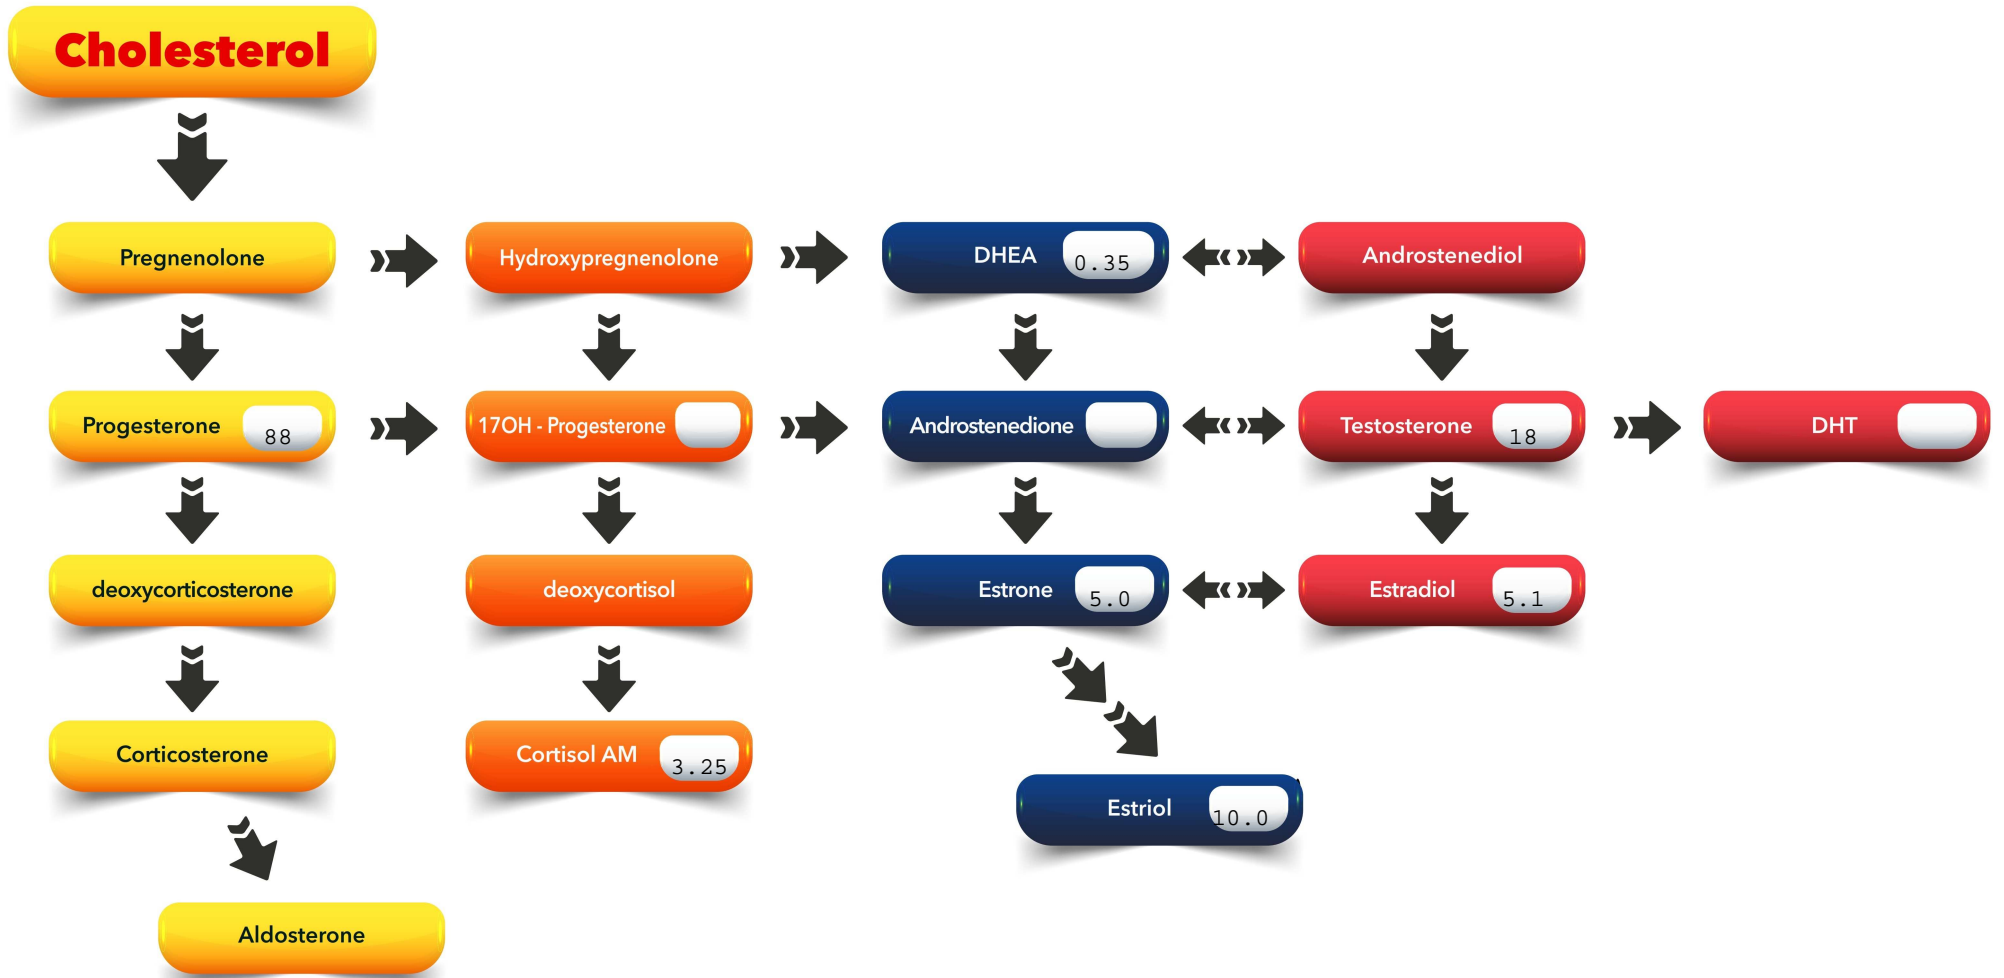

Date of Service: 09/11/19 12:12
 Patient Name: TEST, PATIENT
 D.O.B: 02/05/1985
 Age: 34